

This Page Is Inserted by IFW Operations  
and is not a part of the Official Record

## **BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS


**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning documents *will not* correct images,  
please do not report the images to the  
Image Problem Mailbox.**




TITLE: HANDLE FOR ENDOSCOPIC DEVICE  
FIRST NAMED INVENTOR: Christopher Hess  
APP#:  
ATTY: Gerry Gressel TEL. #: 513-337-3535  
DOCKET #: END-5212 CUST. #: 000027777

1/14

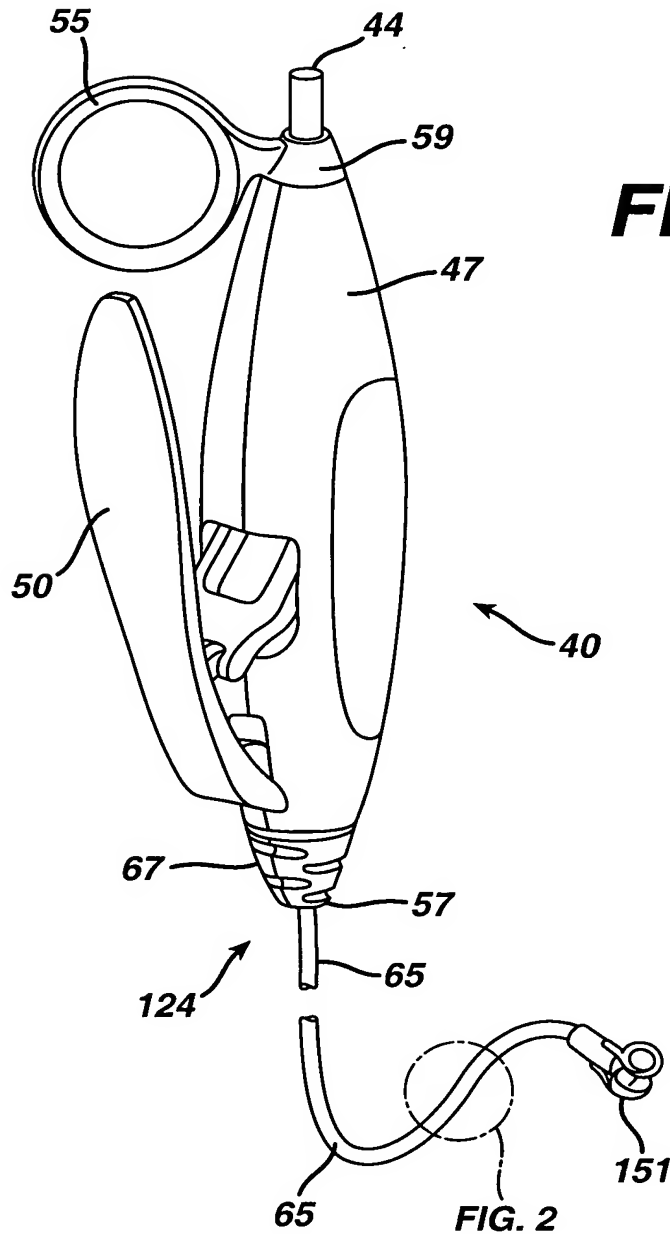


2/14


**FIG. 2**



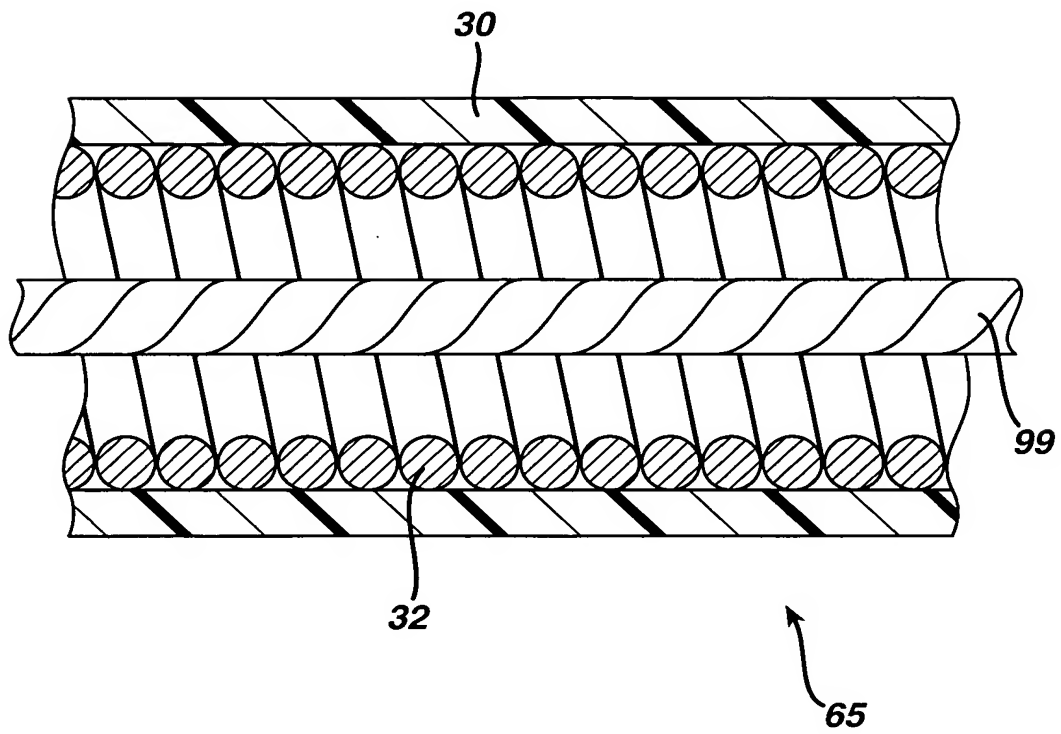


3/14

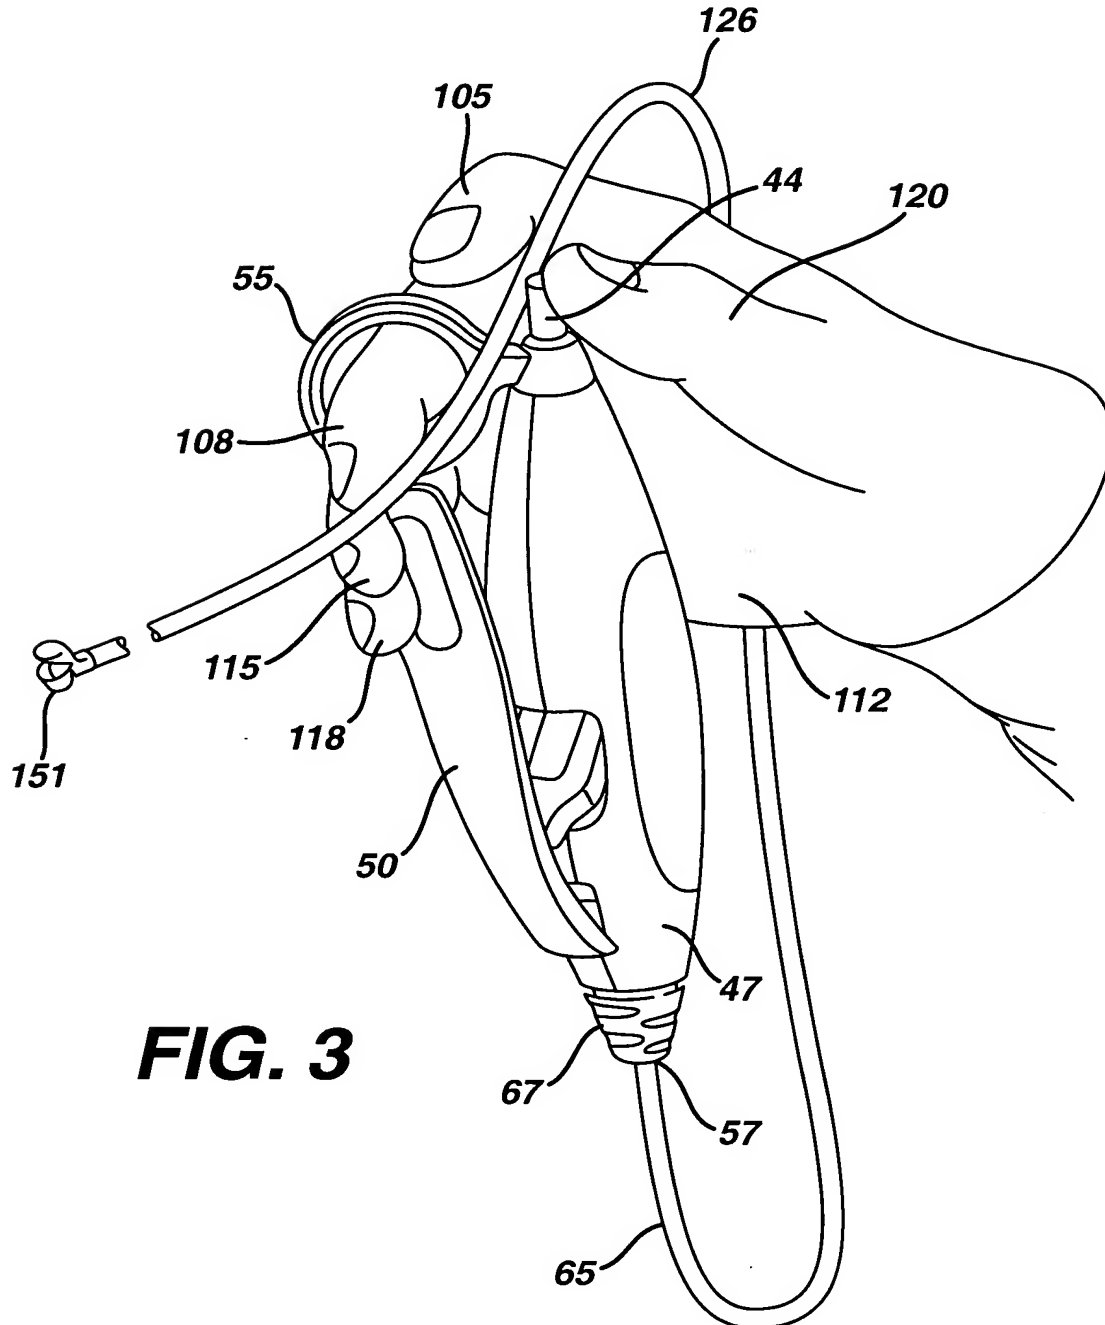


4/14

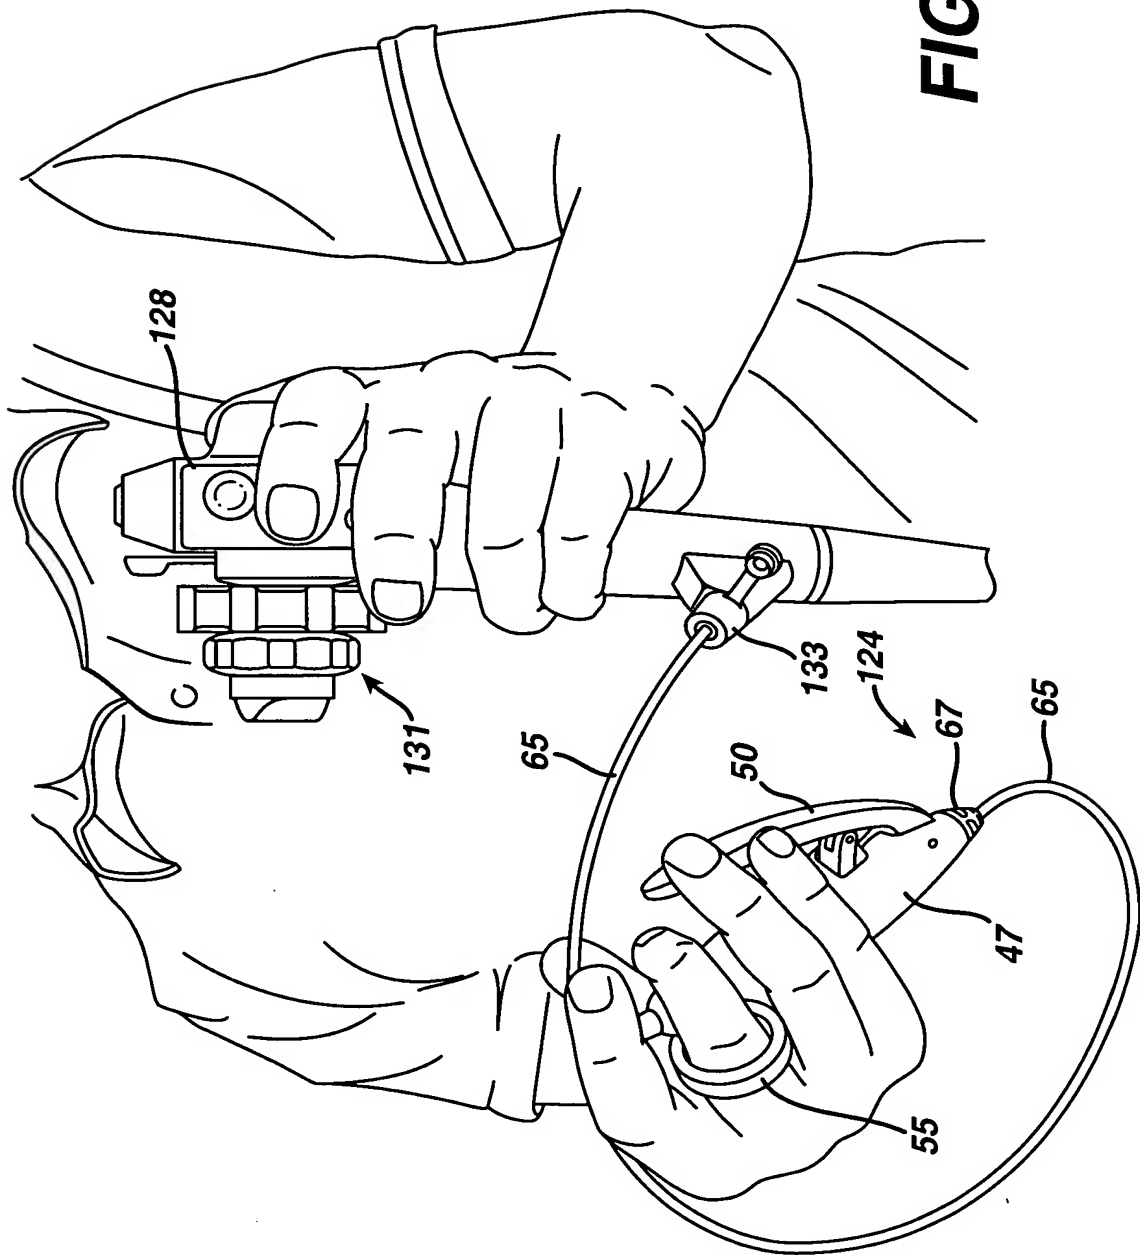

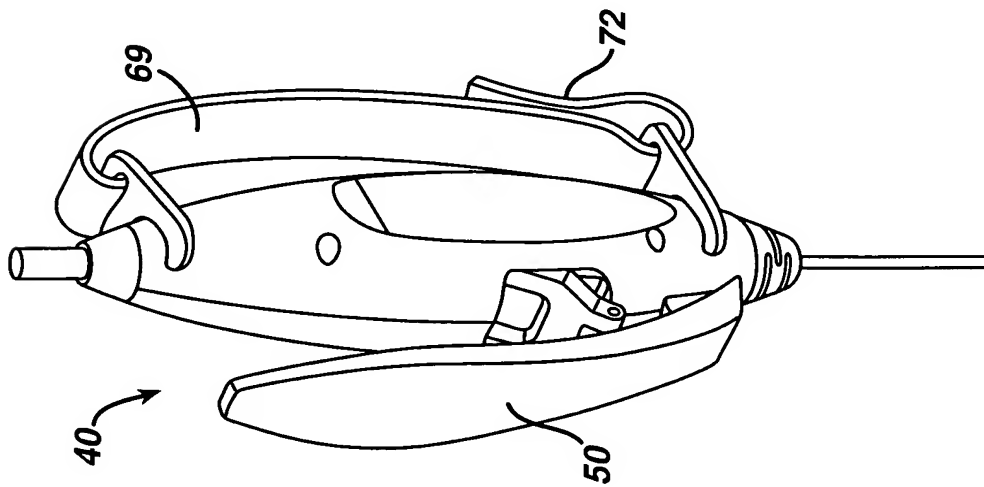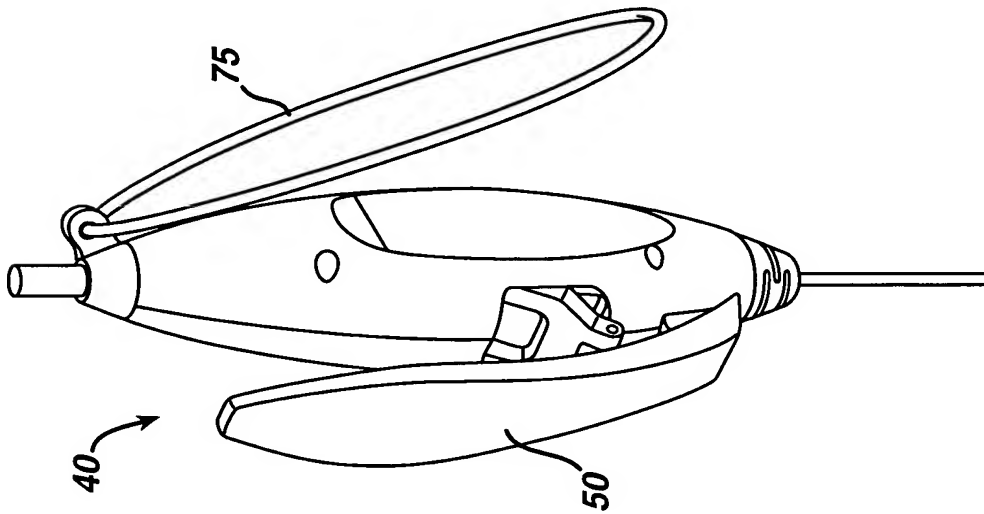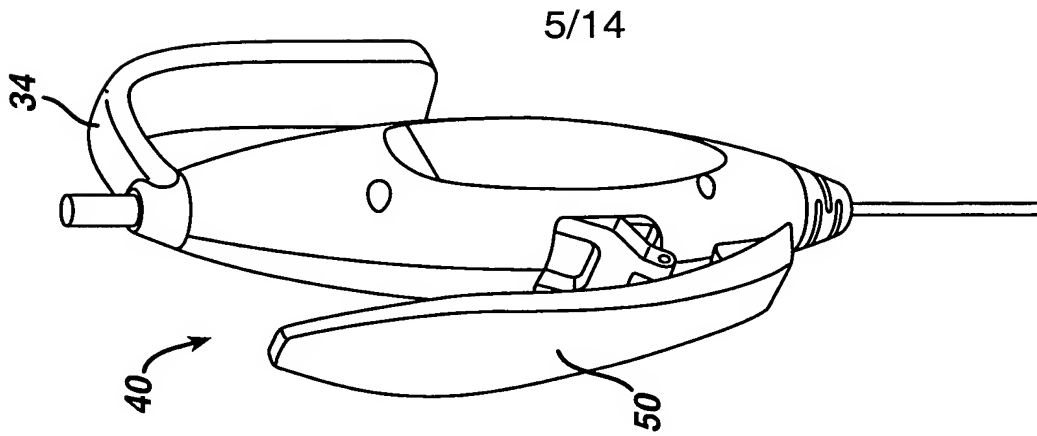


6/14

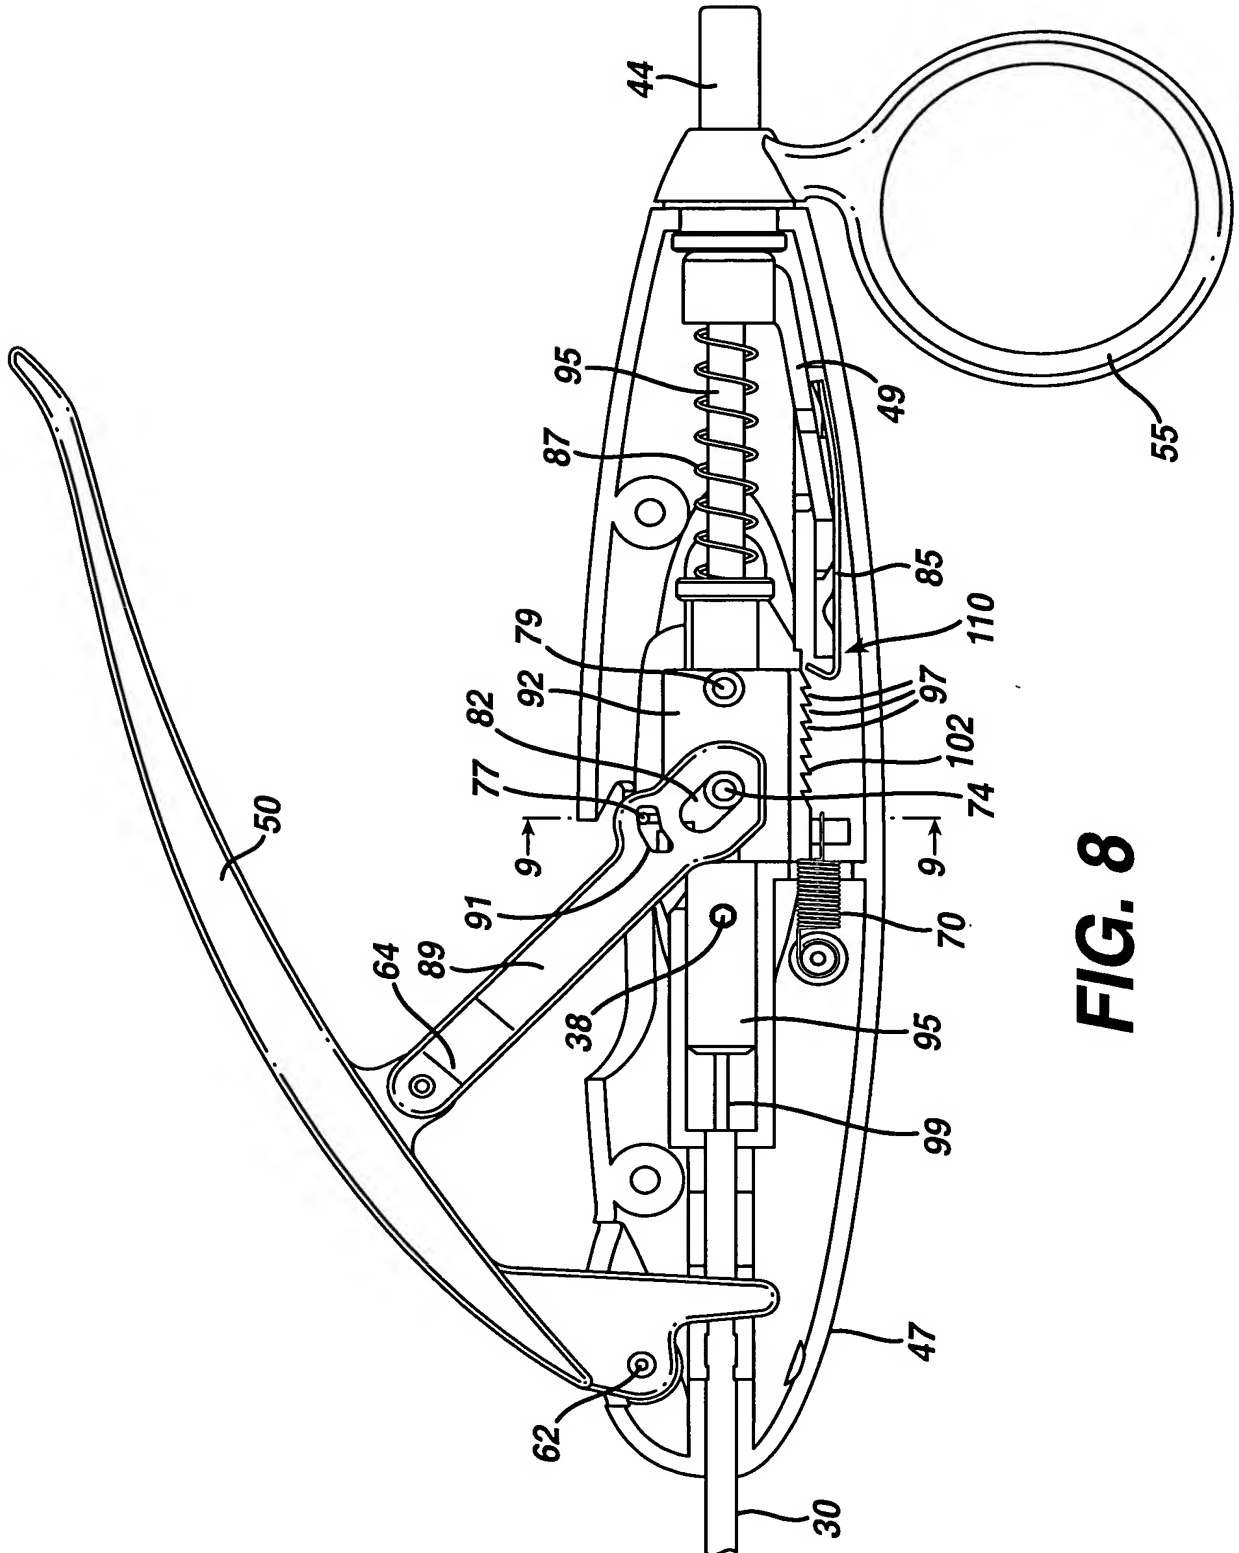


**FIG. 8**

7/14

**FIG. 9**

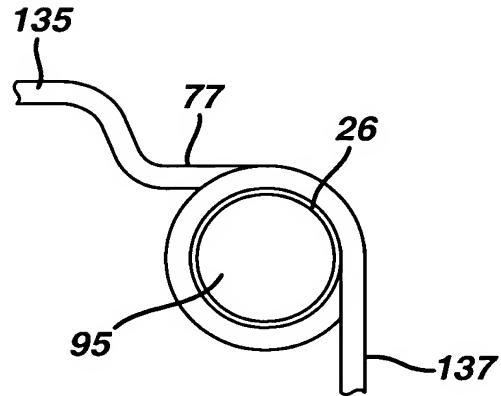


**FIG. 11**

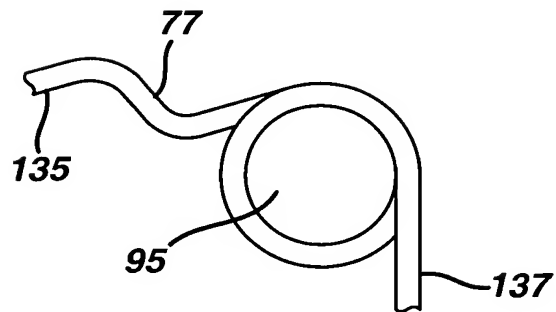





8/14

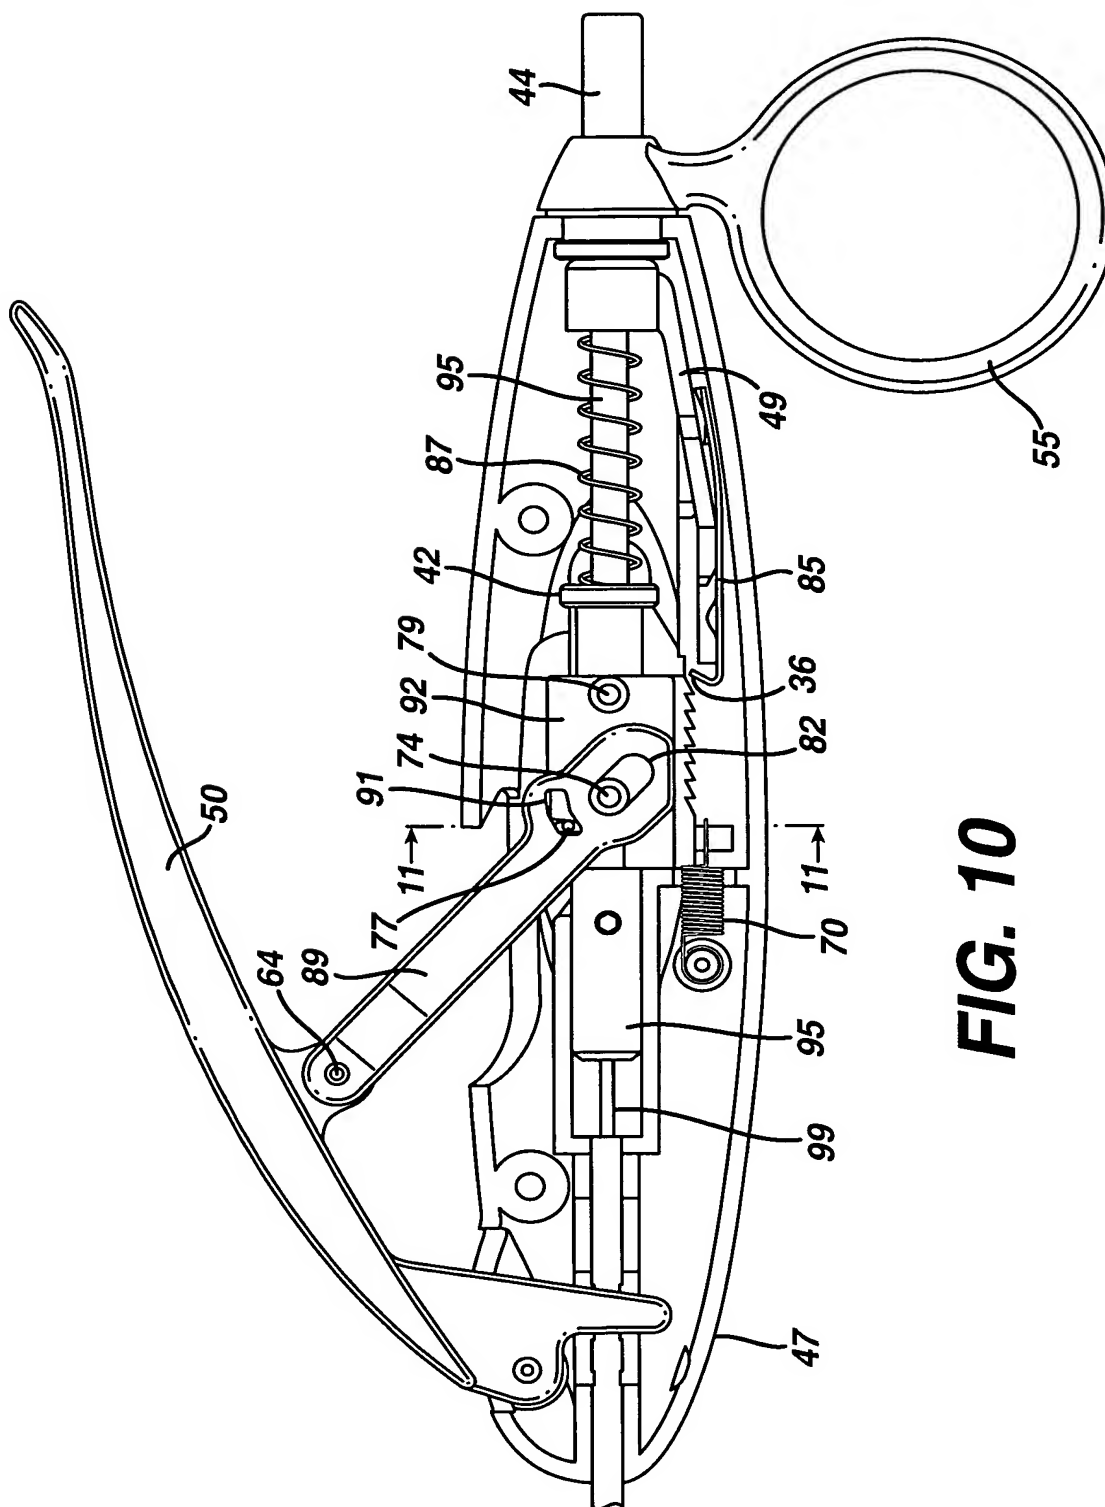


**FIG. 10**

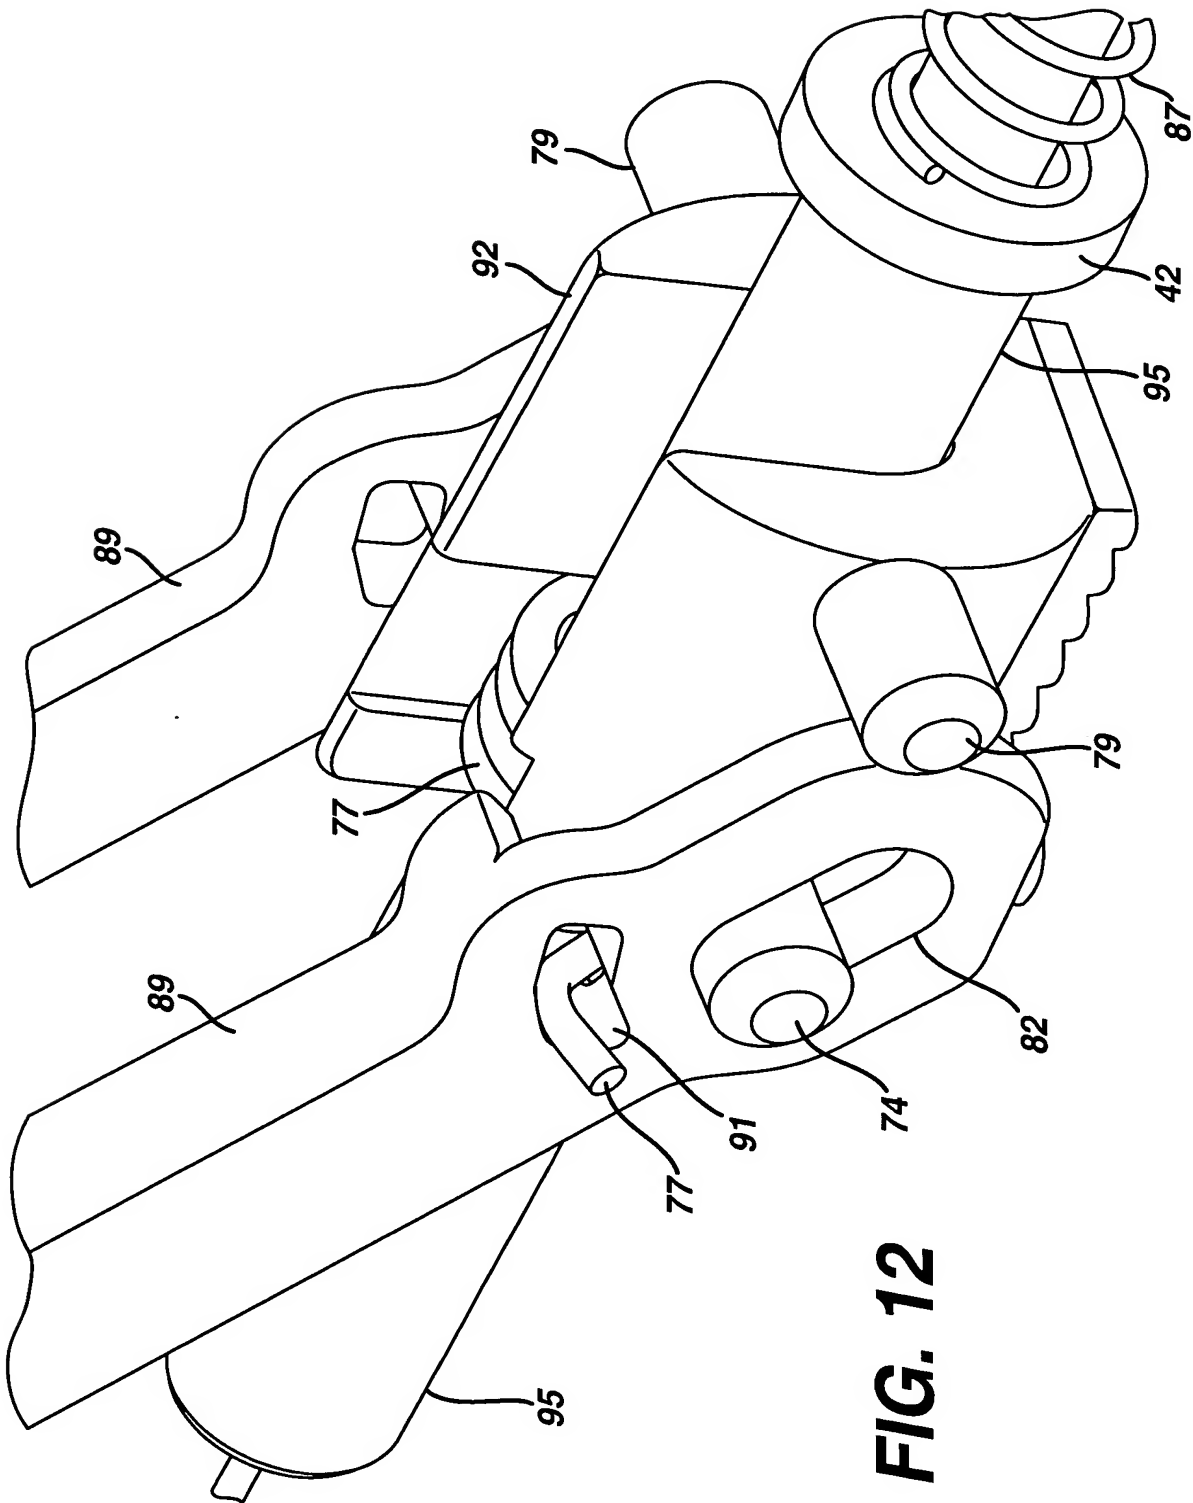

10/14

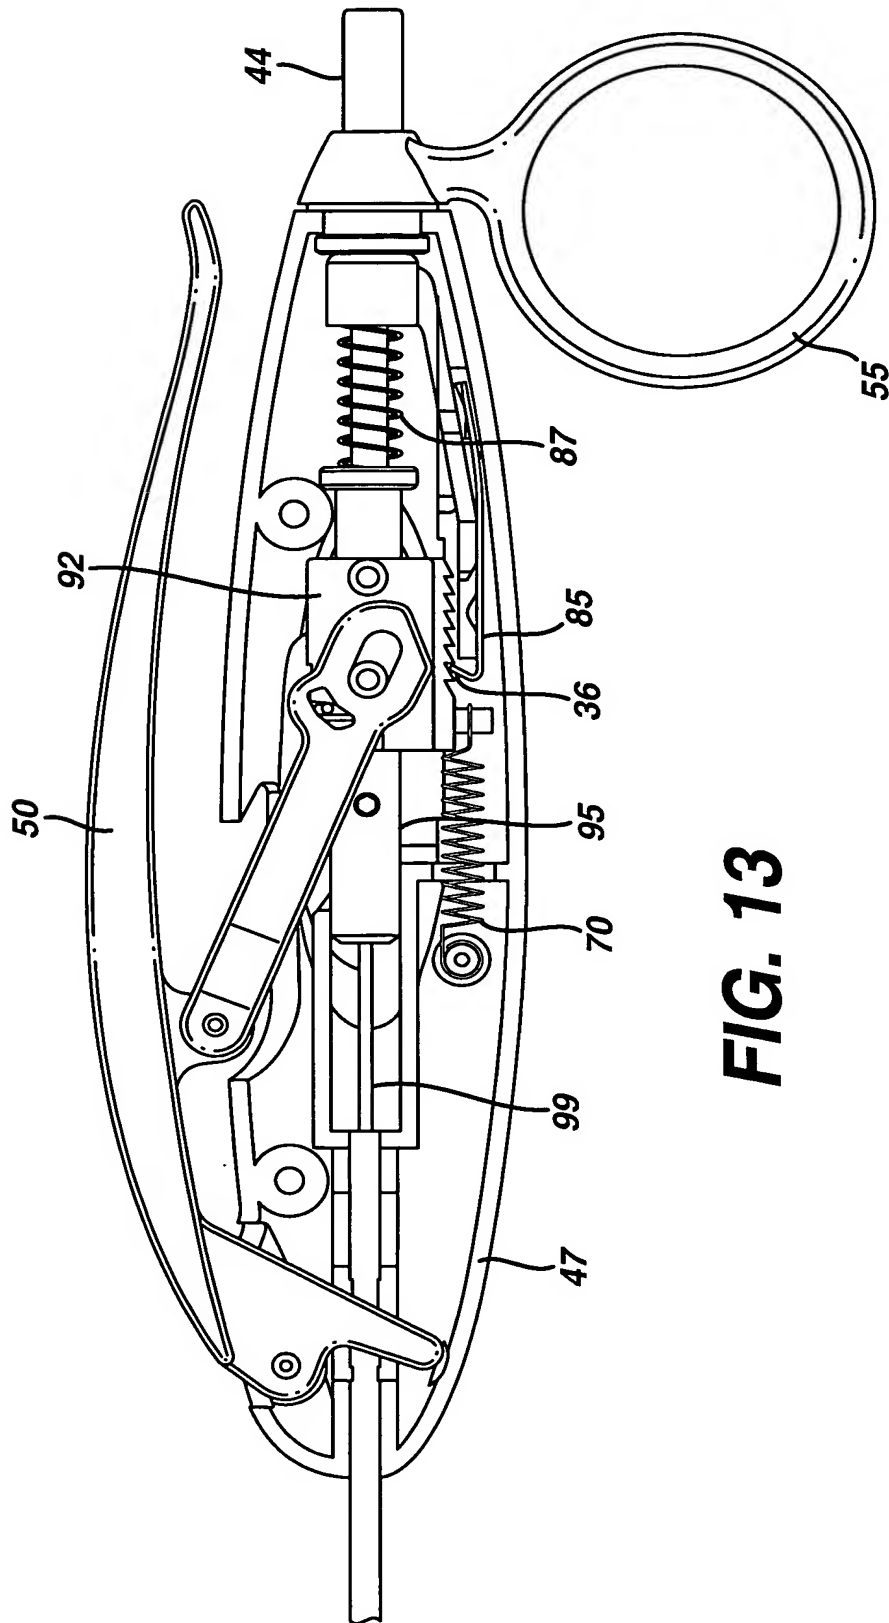


11/14

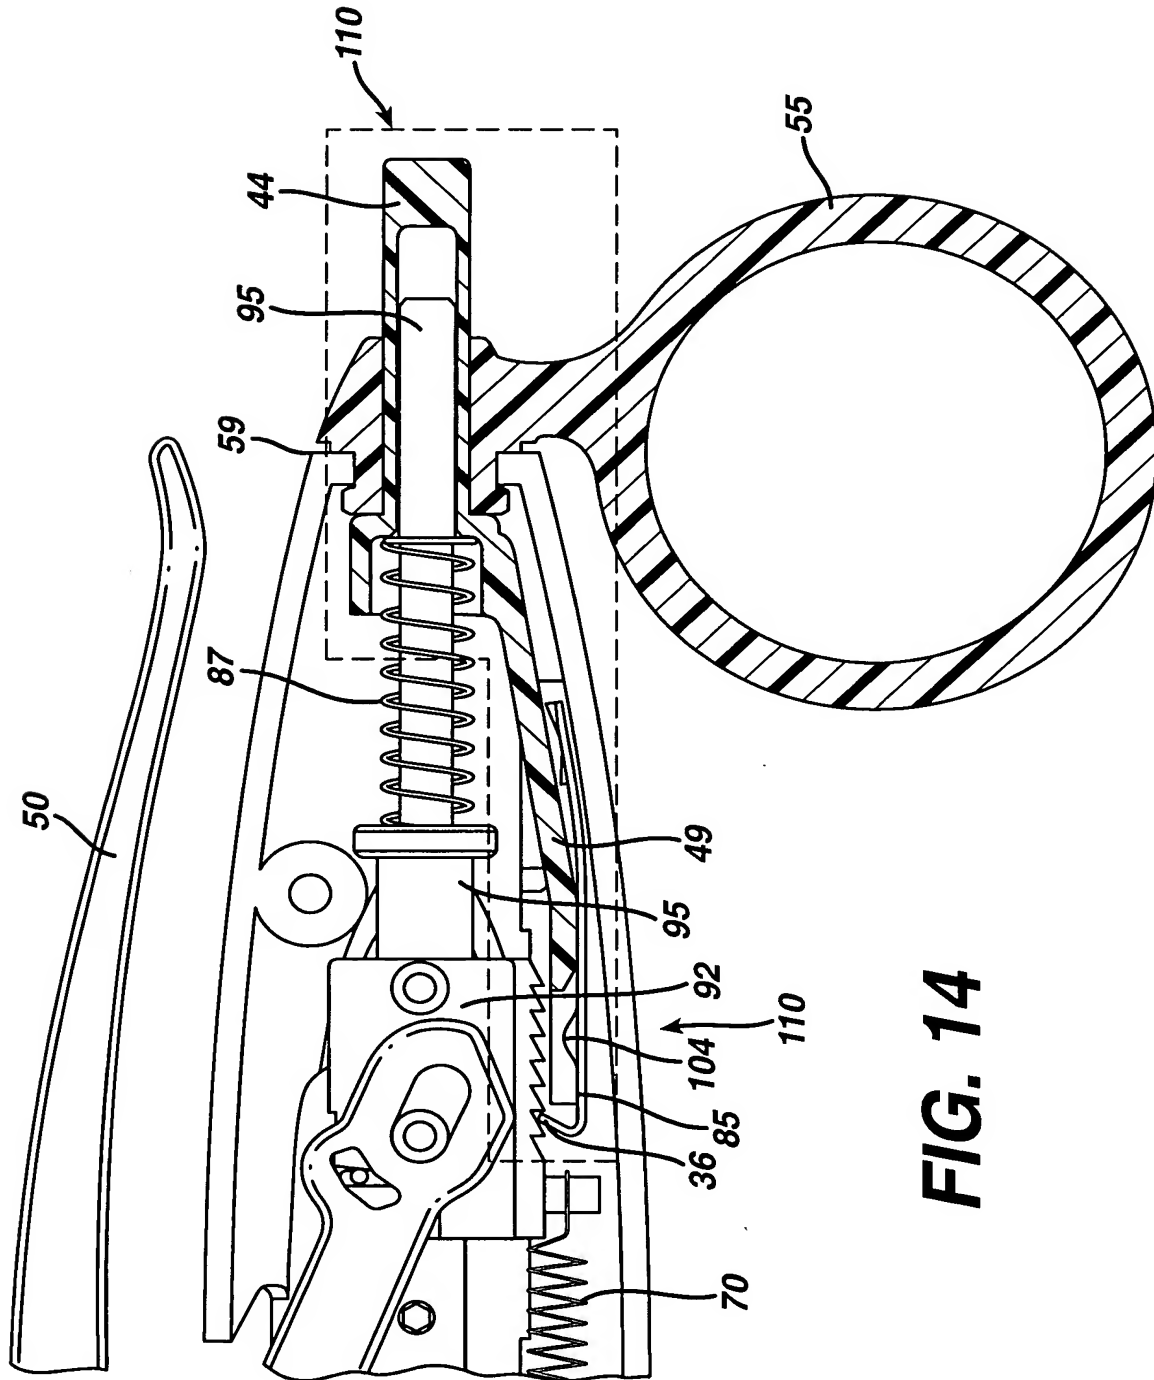


12/14

**FIG. 16**

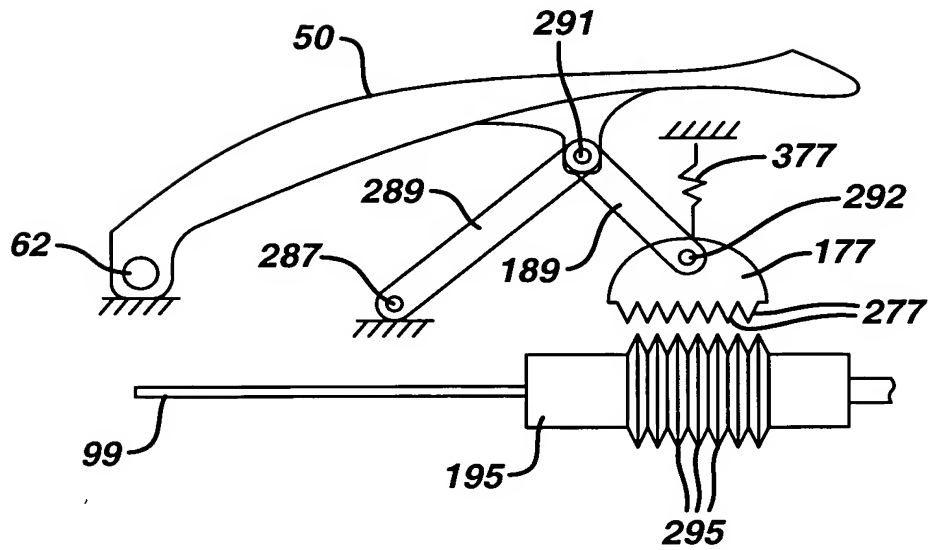


13/14

FIG. 17

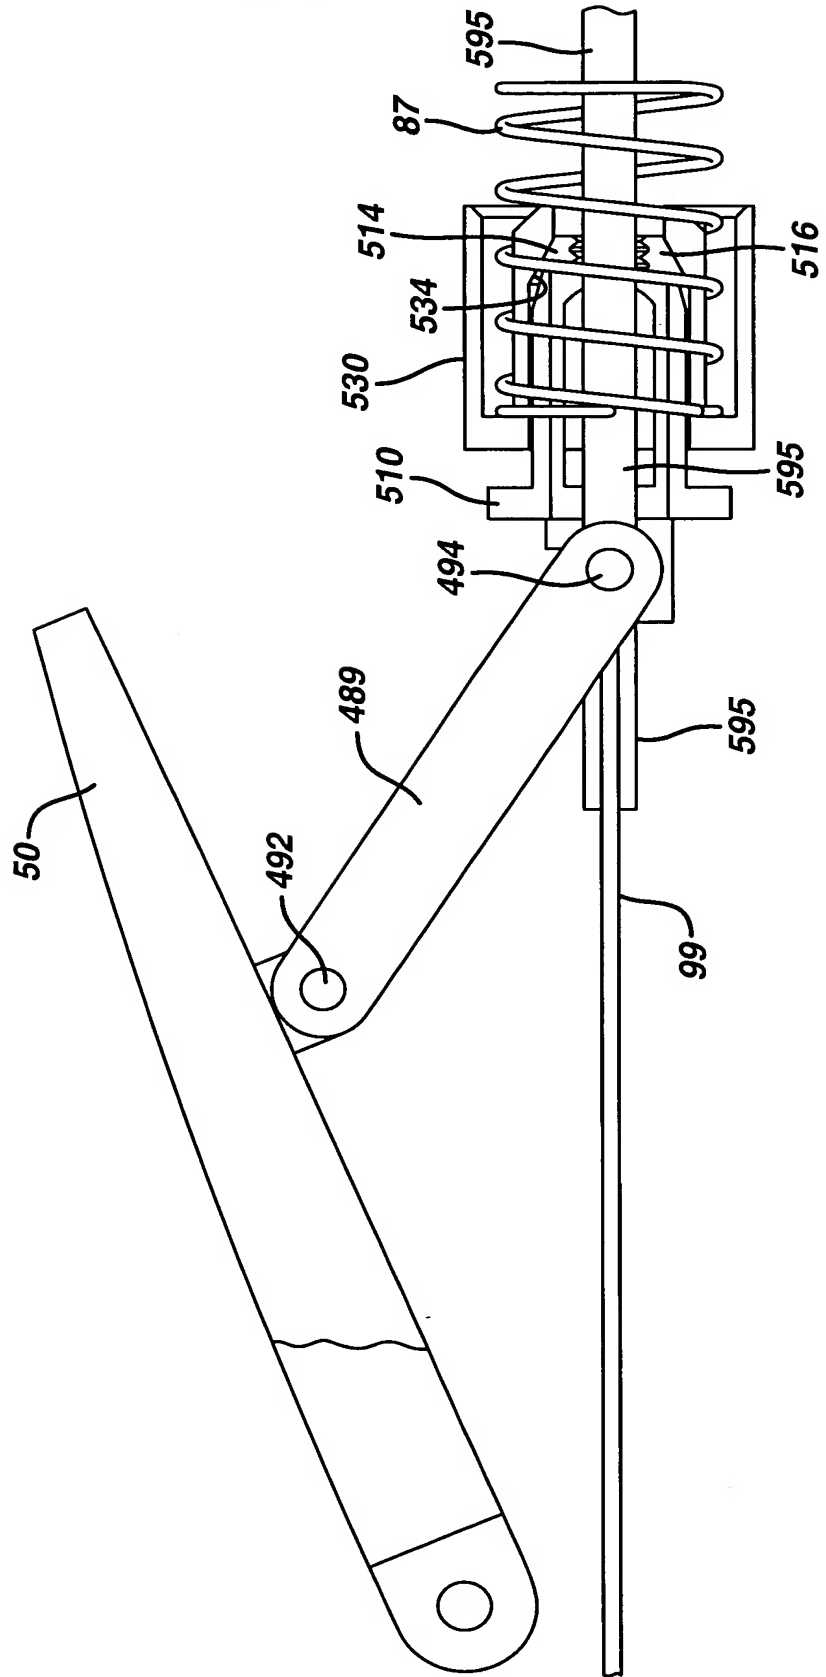


14/14


**FIG. 15A**




**FIG. 15B**




**FIG. 15C**




**FIG. 15D**




**FIG. 15E**




**FIG. 15F**



**FIG. 15G**



**FIG. 15H**



**FIG. 15I**

